

EOG Single Switch Morse code Translate Input Device for Individuals with The Motor Neuron Disease

Chung-Min Wu¹ Ke-Guei Huang¹ Shei-Hsi Chang² Shu-Ching Hsu³ Ching-Ling Lin⁴

¹ Department of Electronic Engineering
Kun-Shan University, Tainan Hsien 710, Taiwan, ROC

² Department of Information and Communication
Kun-Shan University, Tainan Hsien 710, Taiwan, ROC

³ Department of Special Education
National University of Tainan, Tainan 70101, Taiwan, ROC

⁴ Department of Electrical Engineering
National Cheng Kung University, Tainan 70101, Taiwan, ROC

Abstract- This study purposes to provide EOG single switch Morse code translate input device for individuals with the Motor Neuron Disease, such as Amyotrophic Lateral Sclerosis. In this study, the unstable signal is transformed to standard logic level by EOG baseline tracing algorithm in the Microprocessor, and the outputs unstable Morse code sequences are recognized by the sliding fuzzy recognition algorithm. The results demonstrate the unstable Morse code sequences can recognize successful by the sliding fuzzy algorithm and translated into readable characters. The disabled can input Morse code with their eyes to operate the computer and household appliances, such as lamps, fans, TV. Therefore, this study provides a useful assistive tool for a user with the Motor Neuron Disease to communicate with the general public.

Keywords: EOG, Morse code, Motor Neuron Disease, Amyotrophic Lateral Sclerosis, assistive tool

I. INTRODUCTION

With the progress of information era, there are many assistive tools developed for the disabled to interact with their environment. However, the Morse code is an efficient tool [10] for the severe disabilities such as the Motor Neuron Disease (MND) and the spinal cord injures. The Morse code is always used to represent various characters by a series of long-short tones. Now, there are many forms of switch to input Morse code, the user can select a fit and comfortable switch such as a single switch (the blow type and the bite type etc.) [11]. But a user must remember the miscellaneous Morse code and accept an exacting training on the stable typing speed with a fixed long-to-short ratio. To keep a fixed input speed that is difficult for the disabled people. In order to release the serious limitation of typing speed control, several algorithms were proposed to chase the typing pattern of a user. After 1995, there are several algorithms [1-9] proposed for unstable input speed by using adaptive and network signal processing techniques including adaptive unstable-speed prediction (AUSP)[1], least mean square and matching (LMS&M)[2], adaptive variable-ratio threshold prediction (AVRTP)[3, 4], the back propagation neural network (BPN)[5, 6], and fuzzy algorithms (e.g. fuzzy recognition [7, 8]). The recognition rate of unstable typing

pattern had significant improvement from AUSP algorithm (29.1%), LMS&M algorithm (81.6%) to AVRTP algorithm (94.0%)[4]. It is successful to solve the problem of the irregular input speed, but the mathematic computation becomes more and more complex, except fuzzy algorithm can be installed in the single-chip microprocessor as real time recognition for a portable device.

This study purposes to provide a novel Morse code assistive input device for individuals with the Motor Neuron Disease, such as Amyotrophic Lateral Sclerosis (ALS), we named "EOG Single switch Morse code Translate input device (ESMcTin)". ESMcTin includes two parts that are EOG switch and Morse code automatic recognition algorithm. In EOG switch, ESMcTin measurements the Electro-Oculography (EOG) signal and translated into Morse code signal by the baseline tracing algorithm. In Morse code automatic recognition algorithm, we use fuzzy theory combining with the signal processing (ie. the sliding window average algorithm) to recognize Morse code and translated into readable characters. This recognition algorithm process its simple and fast-speed calculation is easily installed in the single-chip microprocessor as real time recognition, and the signal processing algorithm can modify the unstable Morse code sequences to more stable sequences for raising the recognition rate of Morse code. The user can input Morse code by their eyes moving through ESMcTin to operate the computer and household appliances, such as lamps, fans, TV. Therefore, this study can provide a useful assistive tool for a user with the Motor Neuron Disease to communicate with the general public.

II. METHOD

In this study, we divide ESMcTin into EOG single switch and Morse code automatic recognition algorithm. The structure of ESMcTin shown in Fig. 1.

$$F_T \begin{cases} x_k = I_k, & \text{if } I_k < T_k \\ x_k = \frac{1}{LSR} I_k, & \text{if } I_k \geq T_k \end{cases} \quad (1)$$

Where T_k is the k th threshold to distinguish between long and short elements.

- To reduce the difficulty in maintaining a stable input rate and increase the stability of signal processing, the sliding window averaging technology is used to chase the variation of long-to-short ratio. The following adopts two windows which have five data (w_{lb} , w_{sb}) where lowercase 'l' and 's' refer to the sliding window of long and short elements respectively, and the lowercase 'b' is the position of input data put in the sliding window, and calculate the average of long and short elements (L_m , S_m) respectively,

When input data I_k is long element,

$$w_{lb} = w_{lb-1}, \quad lb = 5, 4, 3, 2 \quad (2)$$

$$w_{l1} = I_k \quad (3)$$

$$L_m = \frac{\sum_{k=1}^5 w_{lk}}{5} \quad (4)$$

Otherwise,

$$w_{sb} = w_{sb-1}, \quad sb = 5, 4, 3, 2 \quad (5)$$

$$w_{s1} = I_k \quad (6)$$

$$S_m = \frac{\sum_{k=1}^5 w_{sk}}{5} \quad (7)$$

Then

$$LSR = \frac{L_m}{S_m} \quad (8)$$

- The prediction error e_k , an input to the fuzzy algorithm, is created by the difference between x_k and y_{k-1} ,

$$e_k = x_k - y_{k-1} \quad (9)$$

To obtain e'_k , a linguistic fuzzy rule is the same as shown in the one-node fuzzy recognition algorithm.

- Based on the values of e'_k and y_{k-1} , the predictive output y_k and threshold T_k are updated by

$$y_k = y_{k-1} + e'_k \quad (10)$$

$$T_k = \frac{LSR + 1}{2} y_{k-1} \quad (11)$$

By repeating steps 1~4, the system can automatically adjust the threshold value (T_k) in response to the typing speed variation and the varying ratio of long to short element.

T_k is $\frac{LSR + 1}{2}$ times of y_{k-1} (i.e., the middle value of between long and short elements). The look-up table in Fig. 3(a) is used to translate Morse codes into readable characters.

III. RESULT AND DISCUSSION

This section presents the test result of the EOG single switch and Morse code automatic recognition algorithm, and the clinical application.

A. The output of the EOG single switch

Fig. 4 is the output of the EOG single switch, Fig. 4(a) is the digital signal of the original EOG signal by ADC, and Fig. 4(b) is the output of EOG single switch by baseline tracing algorithm. When the user input Morse code by the eyes, the level of signal has the drift, but the baseline tracing algorithm can trace the baseline variation of EOG signal in the static state, such as Fig. 4(a) and output the correct Morse code signal such as Fig. 4(b).

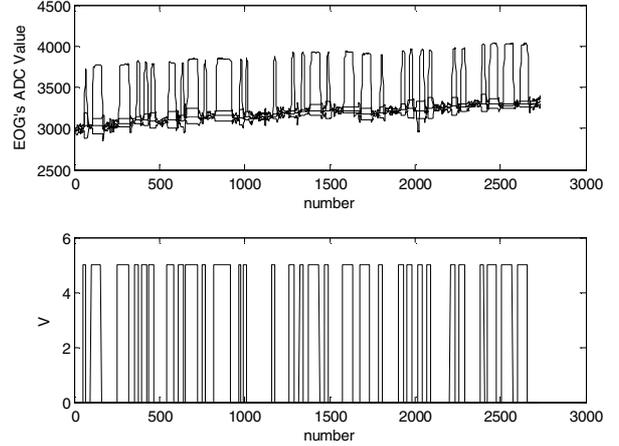


Fig. 4 The output signal of EOG single switch

B. The performance of Morse code recognition algorithm

We designed a simulation data to test the performance of Morse code recognition algorithm (i.e., the sliding fuzzy recognition algorithm). Simulation data is a Morse code sequence in an alphabetic order from a to z with a sinusoidal speed variation for the user's typing variation (fast or slow). In simulation of data that the long element is set at 300msec, the short element is set at 100msec, and the variation of sinusoidal is 100msec in the Morse code sequence (the variation of the long-to-short ratio is about from 3:1 to 2:1). Fig. 5 is the sliding fuzzy recognition result that can adjust the threshold value between long and short elements correction in quick motion and have a successful recognition for long-to-short ratio variation from 3:1 to 2:1.

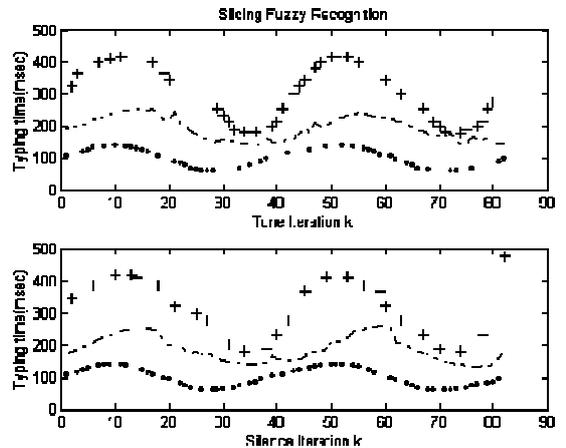


Fig. 5 Recognition result with simulation data by the sliding fuzzy algorithm

C. The clinical application

The user used the specially designed EOG single switch to input the appropriate Morse code elements for alphanumeric characters. The corresponding characters were then presented to him on a computer monitor in real time. This study presents the result of ten times typing test from two subjects that they are both beginner of Morse code. The subject's typing patterns and speeds when typing the ten letters (a to j) of the English alphabet were recorded, the average recognition rate about 98% and spends between 48 and 69 seconds.

IV. CONCLUSIONS

In this study, the unstable signal is transformed to standard logic level by EOG baseline tracing algorithm in the Microprocessor. And then the outputs unstable Morse code sequences are recognized by the sliding fuzzy recognition method. The results demonstrate the unstable Morse code sequences can be recognized successful by the sliding fuzzy algorithm and translated into readable characters.

In the clinical application, the user can input the character stable and correctly by EOG single switch, but the eyes will get tired easily by typing the code with eyes for a long time and making the unstable Morse code sequence. How to improve this defects that is an important subject in future.

Additionally, we will alter the functions of the ESMcTin and enhanced the training of Morse code input depends on the comments of the user. Hope the ESMcTin is a useful assistive communication tool can help the servers disable to communication with others.

ACKNOWLEDGMENT

The National Science Council, Taiwan, Republic of China supported this research, under contract NSC94-2213-E-168-018.

REFERENCES

- [1] C. H. Luo and C. H. Shih, "Adaptive Morse-coded single-switch communication system for the disabled," *International Journal of Bio-Medical Computing*, Vol. 41, pp. 99-106, 1996.
- [2] C. H. Shih and C. H. Luo, "A Morse-code recognition system with LMS and matching algorithms for persons with disabilities," *International Journal of Medical Informatics*, Vol. 44, pp. 193-202, 1997..
- [3] C. H. Luo and M. C. Hsieh, "Morse Code Typing Training of a Teenager with Cerebral Palsy using Microcomputer Technology," *Augmentative and Alternative Communication*, Vol. 15, pp. 1-6, 1999.
- [4] M. C. Hsieh, C. H. Luo, and C. W. Mao, "Unstable Morse code recognition with adaptive variable-ratio threshold prediction for physically disabled persons," *IEEE Trans. Rehab. Eng.*, Vol. 8, No 3, pp. 405-413, 2000.
- [5] D. T. Fuh and C. H. Luo, "Unstable Morse code recognition system with back propagation neural network for person with disabilities," *J. Med. Eng. & Tech.*, Vol. 25, No. 3, pp. 118-123, 2001.
- [6] D. T. Fuh and C. H. Luo, "Unstable Morse code recognition system with Expert-Gating Neural network," *Biomedical Engineering Applications Basis and Communications*, Vol. 14, No. 1, pp. 12-19, 2002.
- [7] C. M. Wu and C. H. Luo, "Morse code recognition system with fuzzy algorithm for disabled persons," *J. Med. Eng. & Tech.*, Vol. 26, No. 5, pp. 202-207, 2002.
- [8] C. W. Tao, and J. Taur, "Design Fuzzy Controllers with adaptive rule insertion. *IEEE Trans. on systems*", *MAN, and Cybernetics-part B: Cybernetics*, vol. 29, no. 3, 1999.

- [9] C. H. Yang, and C. H. Luo, "An Adaptive Algorithm for Morse Code Recognition", *International Journal of The Computer, The Internet and Management*, Vol 7, No. 1: 1-8, 1999.
- [10] C. H. Yang, C. H. Luo, Y. L. Jeang, and G. J. Jon, "A novel approach to adaptive Morse code recognition for disabled persons", *Mathematics and Computers in Simulation* 54:23-32, 2000.
- [11] "Advanced Input Devices" website (<http://www.aac-input.org/english>)